


Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

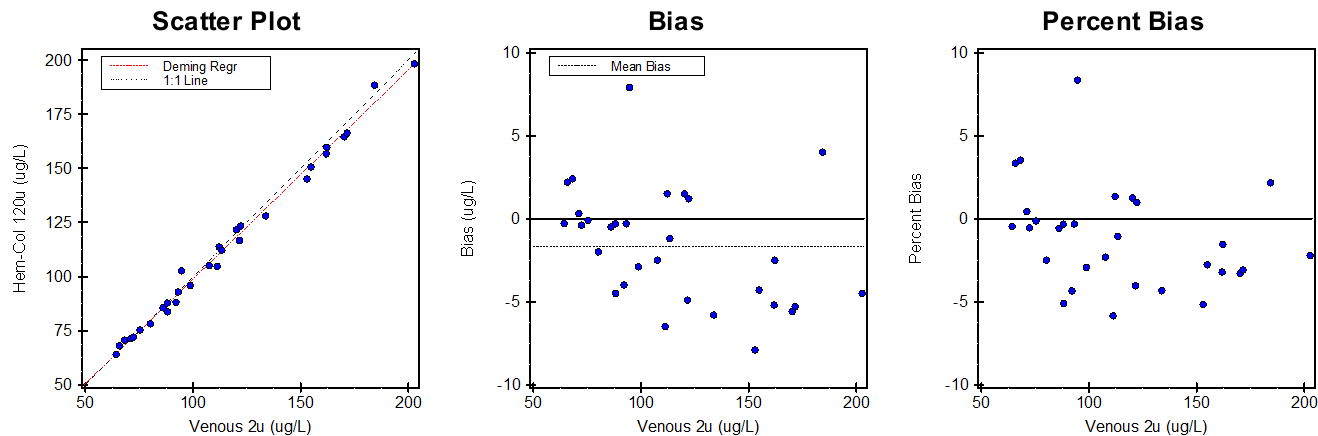

Regression Analysis

	Deming	Regular
Slope	0,966 (0,934 to 0,998)	0,963 (0,931 to 0,994)
Intercept	2,21 (-1,64 to 6,06)	2,60 (-1,25 to 6,44)
Std Err Est	3,27	3,27

95% Confidence Intervals are shown in parentheses

Supporting Statistics

Corr Coef (R)	0,9964	SubRange Bounds	None
Bias	-1,68 (-1,47 %)	Points (Plotted/Total)	30/30
X Mean ± SD	114,73 ± 39,15	Outliers	None
Y Mean ± SD	113,04 ± 37,82	Scatter Plot Bounds	None
Std Dev Diff	3,53		

Experiment Description

	X Method	Y Method
Expt Date	13 jun 2018	13 jun 2018
Rep SD	1	1
Result Ranges	64,3 to 202,8	64,0 to 198,3
Units	ug/L	ug/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: _____

Signature

Date

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	80,2	78,2	-2,0	S00011	68,2	70,6	2,4	S00021	71,1	71,4	0,3
S00002	121,6	116,7	-4,9	S00012	171,6	166,3	-5,3	S00022	64,3	64,0	-0,3
S00003	86,1	85,6	-0,5	S00013	162,2	159,7	-2,5	S00023	88,1	87,8	-0,3
S00004	65,8	68,0	2,2	S00014	98,8	95,9	-2,9	S00024	111,2	104,7	-6,5
S00005	184,4	188,4	4,0	S00015	107,6	105,1	-2,5	S00025	161,9	156,7	-5,2
S00006	154,9	150,6	-4,3	S00016	122,2	123,4	1,2	S00026	153,0	145,1	-7,9
S00007	112,2	113,7	1,5	S00017	88,2	83,7	-4,5	S00027	93,2	92,9	-0,3
S00008	92,1	88,1	-4,0	S00018	133,8	128,0	-5,8	S00028	72,4	72,0	-0,4
S00009	120,2	121,7	1,5	S00019	94,7	102,6	7,9	S00029	202,8	198,3	-4,5
S00010	75,4	75,3	-0,1	S00020	113,4	112,2	-1,2	S00030	170,2	164,6	-5,6

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

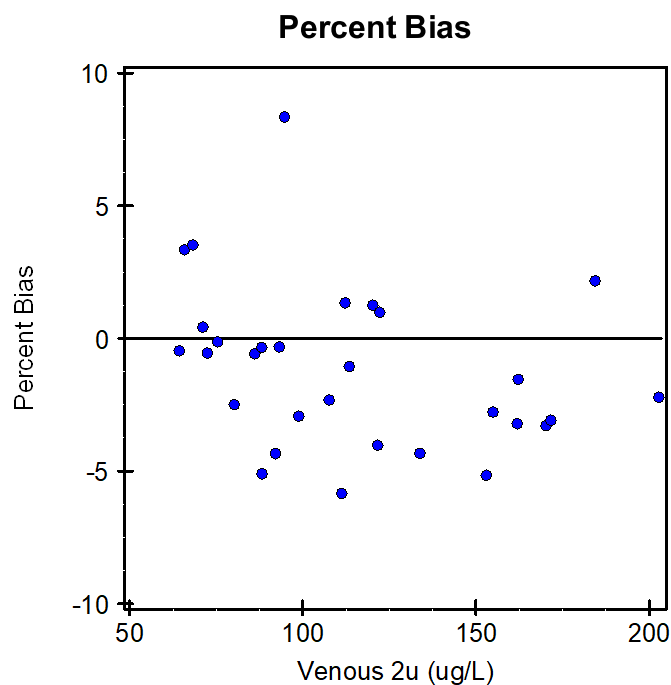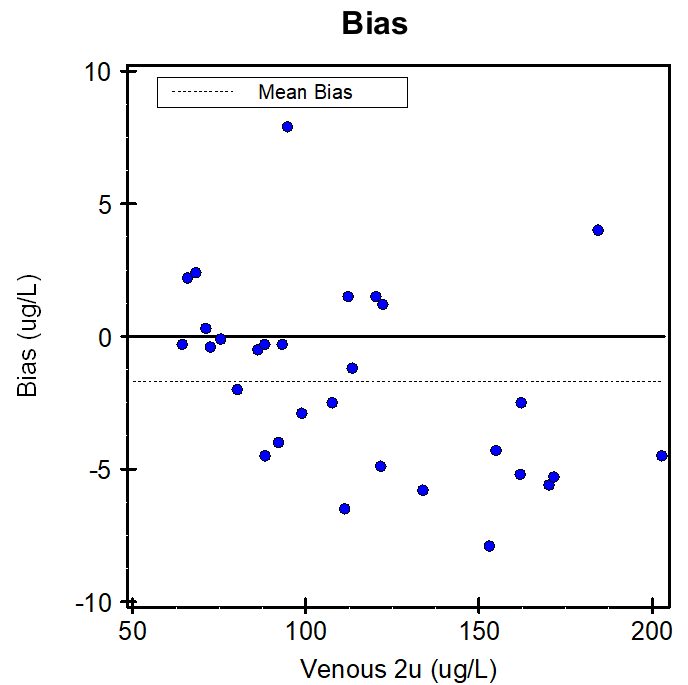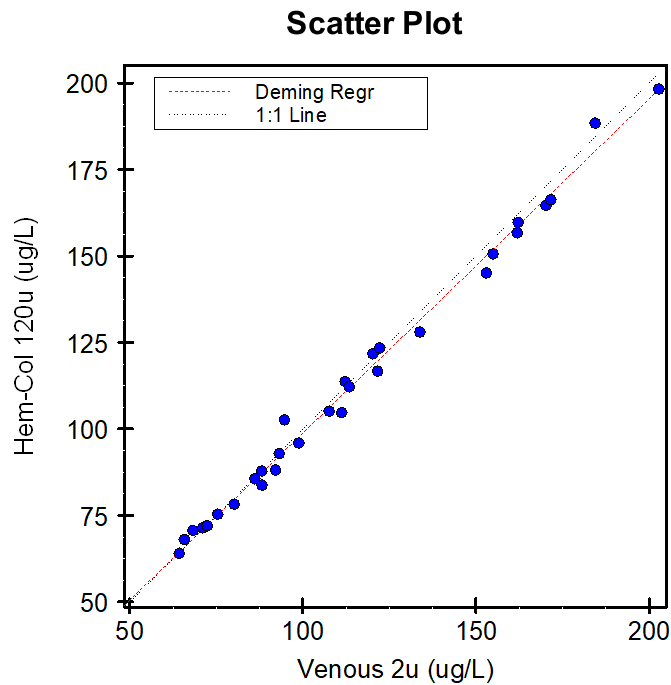

This page contains a larger, working copy of the same graphs that appear on page 1.