


## Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

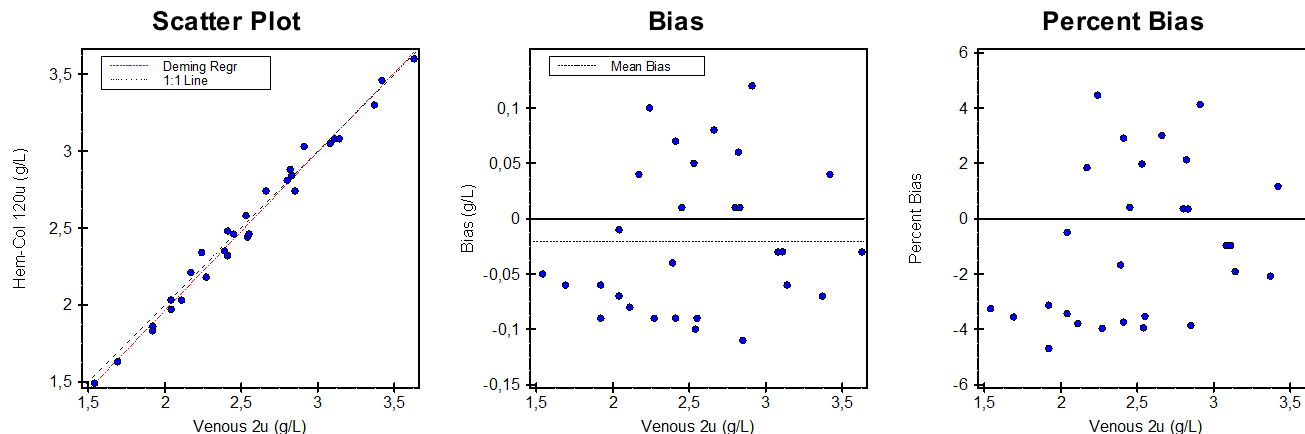

### Regression Analysis

	Deming	Regular
<b>Slope</b>	1,031 (0,983 to 1,079)	1,023 (0,975 to 1,071)
<b>Intercept</b>	-0,099 (-0,224 to 0,026)	-0,079 (-0,204 to 0,045)
<b>Std Err Est</b>	0,065	0,065

95% Confidence Intervals are shown in parentheses

### Supporting Statistics

Corr Coef (R)	0,9927	SubRange Bounds	None
Bias	-0,020 (-0,800 %)	Points (Plotted/Total)	30/30
X Mean ± SD	2,541 ± 0,514	Outliers	None
Y Mean ± SD	2,521 ± 0,530	Scatter Plot Bounds	None
Std Dev Diff	0,065		

### Experiment Description

	X Method	Y Method
Expt Date	13 jun 2018	13 jun 2018
Rep SD	1	1
Result Ranges	1,54 to 3,63	1,49 to 3,60
Units	g/L	g/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: \_\_\_\_\_

Signature

Date

## Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

### Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	1,54	1,49	-0,05	S00011	2,04	1,97	-0,07	S00021	2,39	2,35	-0,04
S00002	2,83	2,84	0,01	S00012	2,82	2,88	0,06	S00022	1,92	1,83	-0,09
S00003	2,04	2,03	-0,01	S00013	2,41	2,48	0,07	S00023	2,85	2,74	-0,11
S00004	2,17	2,21	0,04	S00014	2,55	2,46	-0,09	S00024	2,54	2,44	-0,10
S00005	2,80	2,81	0,01	S00015	3,37	3,30	-0,07	S00025	2,66	2,74	0,08
S00006	1,92	1,86	-0,06	S00016	2,91	3,03	0,12	S00026	2,27	2,18	-0,09
S00007	2,45	2,46	0,01	S00017	1,69	1,63	-0,06	S00027	2,41	2,32	-0,09
S00008	3,14	3,08	-0,06	S00018	3,11	3,08	-0,03	S00028	2,39	2,35	-0,04
S00009	3,63	3,60	-0,03	S00019	2,24	2,34	0,10	S00029	3,08	3,05	-0,03
S00010	2,53	2,58	0,05	S00020	3,42	3,46	0,04	S00030	2,11	2,03	-0,08

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.

### Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

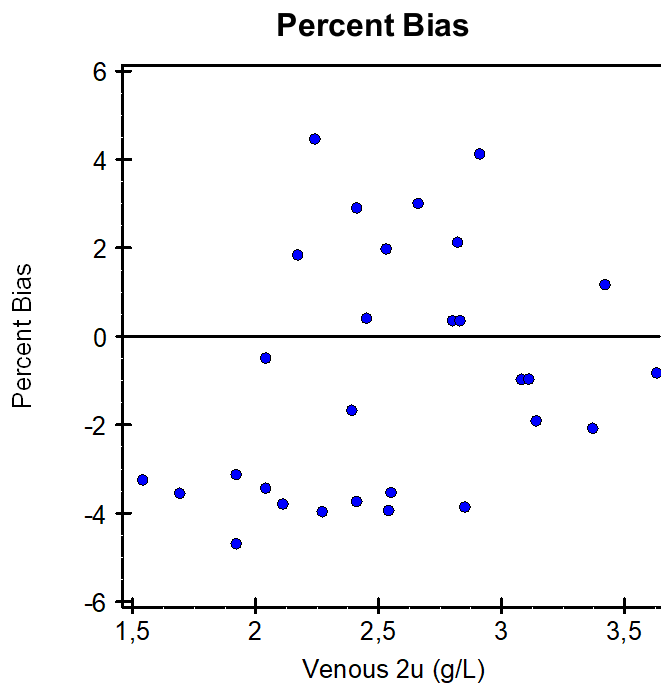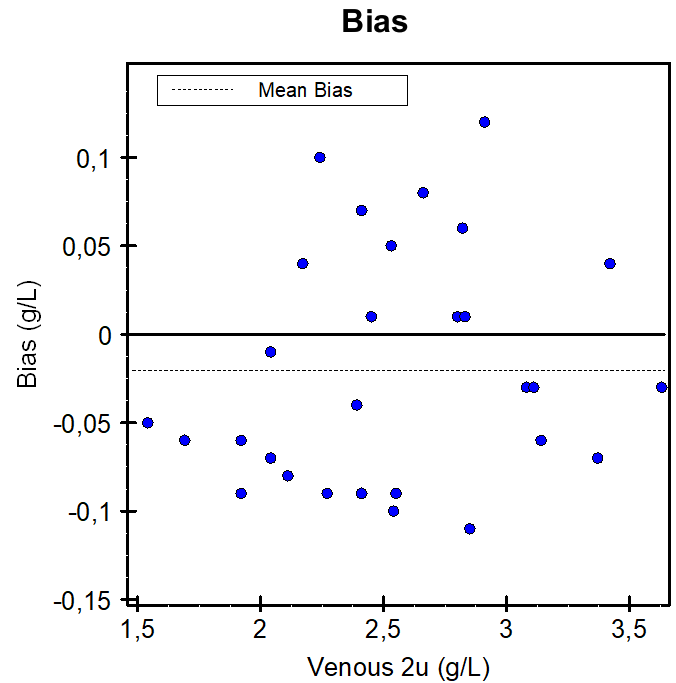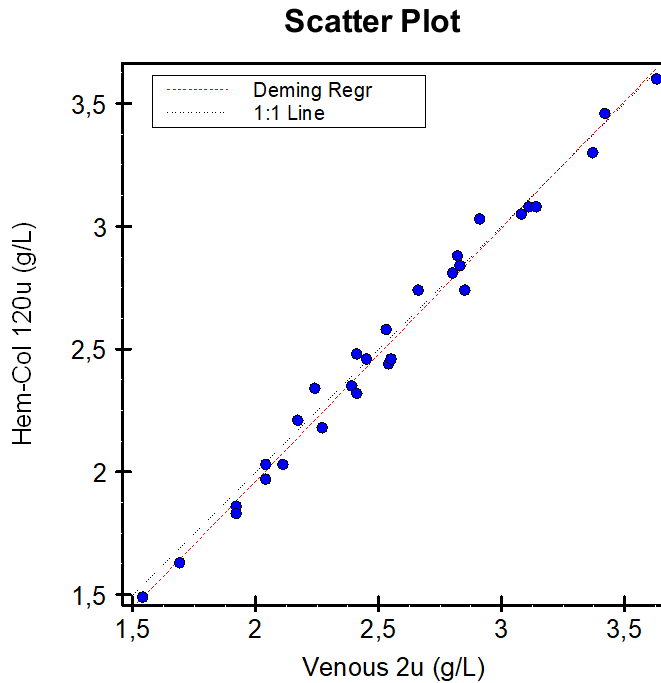

This page contains a larger, working copy of the same graphs that appear on page 1.