


Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

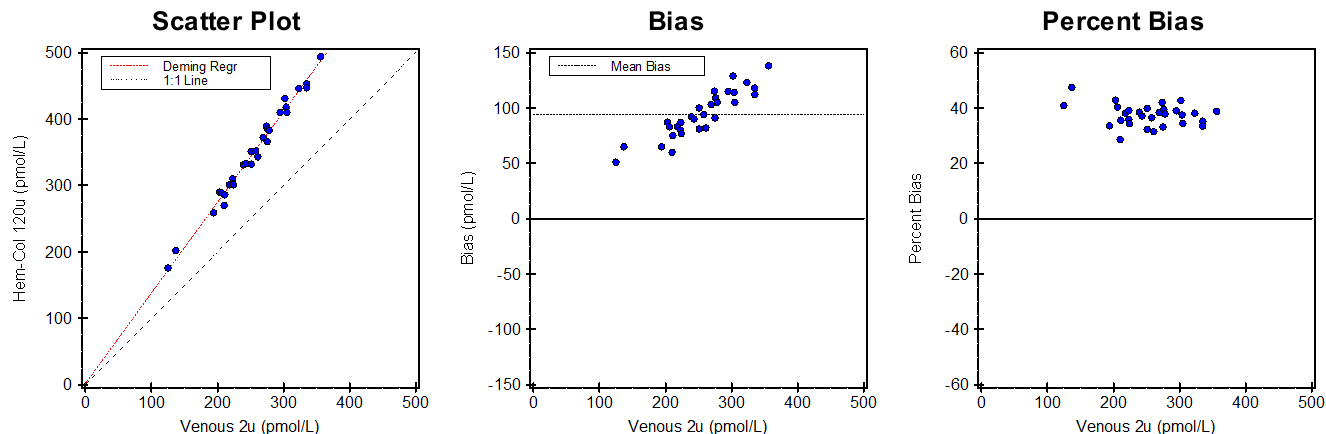

Regression Analysis

	Deming	Regular
Slope	1,365 (1,302 to 1,427)	1,352 (1,290 to 1,414)
Intercept	1,9 (-14,2 to 18,0)	5,0 (-11,1 to 21,1)
Std Err Est	8,9	8,9

95% Confidence Intervals are shown in parentheses

Supporting Statistics

Corr Coef (R)	0,9931	SubRange Bounds	None
Bias	94,3 (37,2 %)	Points (Plotted/Total)	30/30
X Mean ± SD	253,5 ± 54,7	Outliers	None
Y Mean ± SD	347,8 ± 74,4	Scatter Plot Bounds	None
Std Dev Diff	21,2		

Experiment Description

	X Method	Y Method
Expt Date	13 jun 2018	13 jun 2018
Rep SD	1	1
Result Ranges	125 to 356	176 to 494
Units	pmol/L	pmol/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: _____

Signature

Date

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	305	410	105	S00011	206	289	83	S00021	210	270	60
S00002	275	366	91	S00012	356	494	138	S00022	194	259	65
S00003	125	176	51	S00013	224	301	77	S00023	251	332	81
S00004	251	351	100	S00014	258	352	94	S00024	261	343	82
S00005	218	301	83	S00015	278	383	105	S00025	335	447	112
S00006	203	290	87	S00016	274	389	115	S00026	211	286	75
S00007	295	410	115	S00017	335	453	118	S00027	243	333	90
S00008	269	372	103	S00018	302	431	129	S00028	276	385	109
S00009	323	446	123	S00019	137	202	65	S00029	239	331	92
S00010	223	310	87	S00020	304	418	114	S00030	223	303	80

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

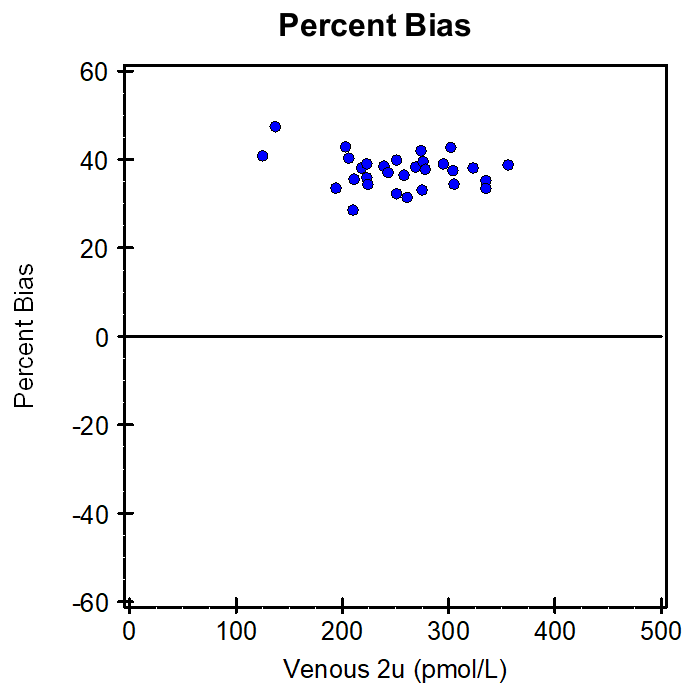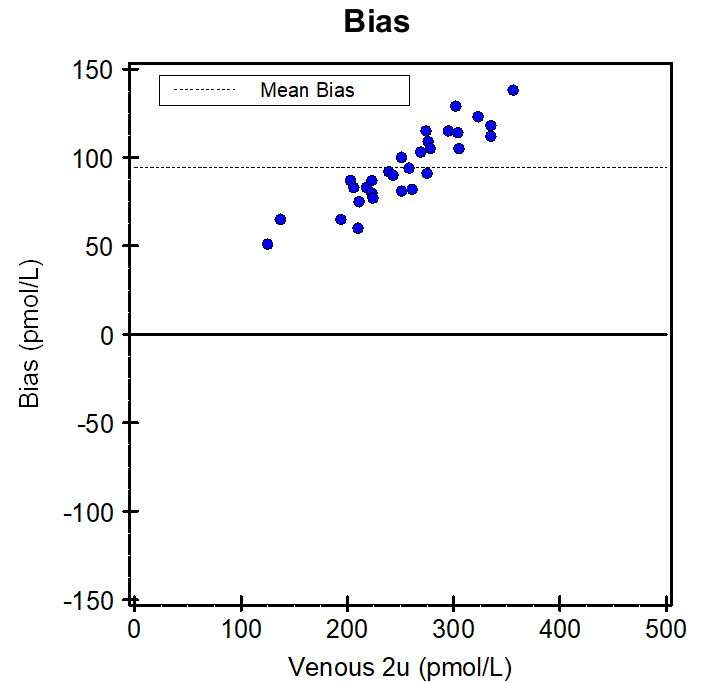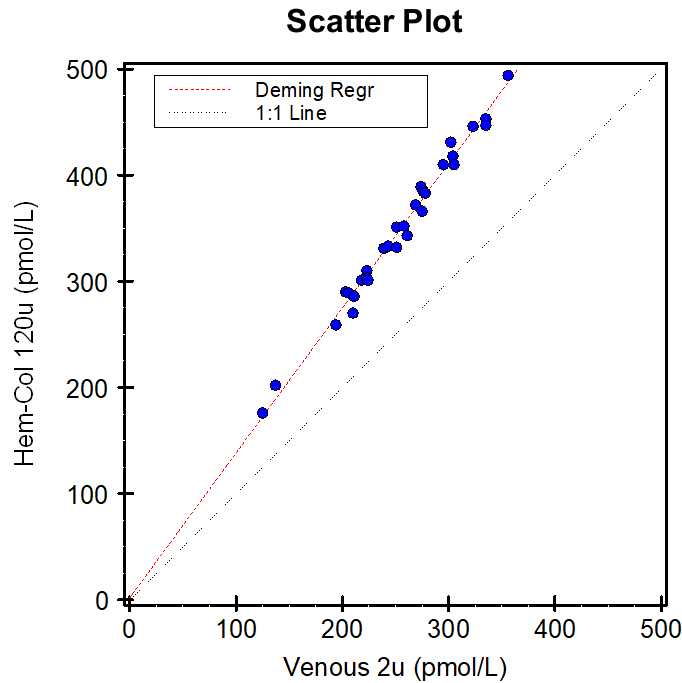

This page contains a larger, working copy of the same graphs that appear on page 1.