
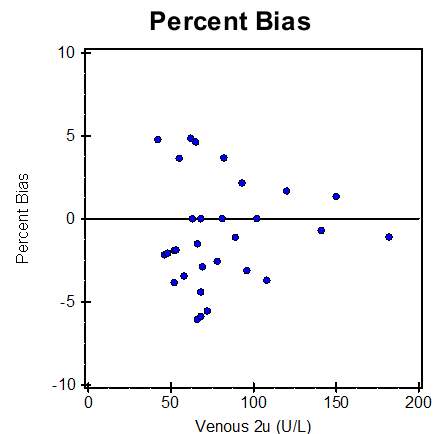
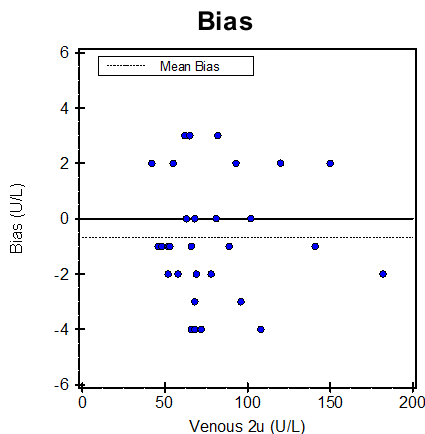


Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

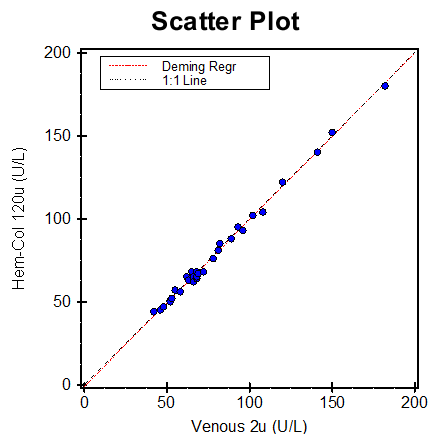

Regression Analysis

	Deming	Regular
Slope	1,003 (0,977 to 1,029)	1,001 (0,975 to 1,027)
Intercept	-0,9 (-3,2 to 1,3)	-0,7 (-3,0 to 1,5)
Std Err Est	2,3	2,3

95% Confidence Intervals are shown in parentheses

Supporting Statistics

Corr Coef (R)	0,9977	SubRange Bounds	None
Bias	-0,7 (-0,8 %)	Points (Plotted/Total)	30/30
X Mean ± SD	79,8 ± 32,8	Outliers	Not Tested
Y Mean ± SD	79,2 ± 32,9	Scatter Plot Bounds	None
Std Dev Diff	2,2		

Experiment Description

	X Method	Y Method
Expt Date	30 mei 2018	06 jun 2018
Rep SD	1	1
Result Ranges	42 to 182	44 to 180
Units	U/L	U/L
Reagent	--	--
Calibrators	--	--
Analyst	R. Huisman	R. Huisman
Comment		

Accepted by: _____

Signature

Date

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	66	65	-1	S00011	150	152	2	S00021	72	68	-4
S00002	46	45	-1	S00012	68	64	-4	S00022	78	76	-2
S00003	66	62	-4	S00013	82	85	3	S00023	58	56	-2
S00004	48	47	-1	S00014	96	93	-3	S00024	42	44	2
S00005	52	51	-1	S00015	65	68	3	S00025	89	88	-1
S00006	53	52	-1	S00016	55	57	2	S00026	93	95	2
S00007	141	140	-1	S00017	102	102	0	S00027	120	122	2
S00008	108	104	-4	S00018	62	65	3	S00028	68	65	-3
S00009	182	180	-2	S00019	68	68	0	S00029	52	50	-2
S00010	81	81	0	S00020	63	63	0	S00030	69	67	-2

Values with an "X" were excluded from the calculations.

Alternate (Quantitative) Method Comparison

X Method Venous 2u

Y Method Hem-Col 120u

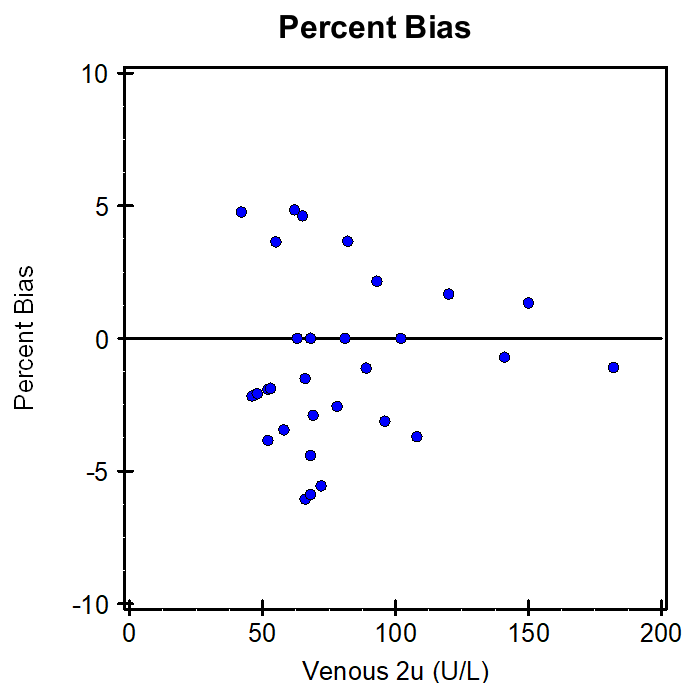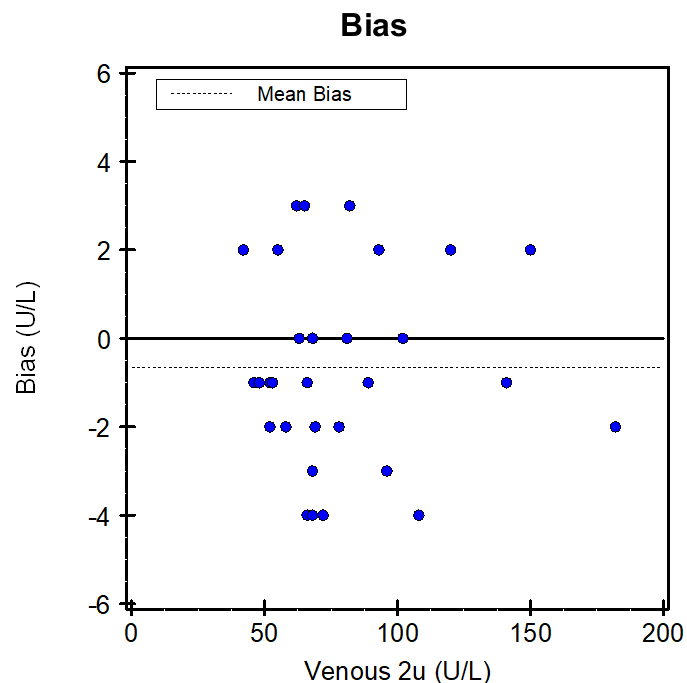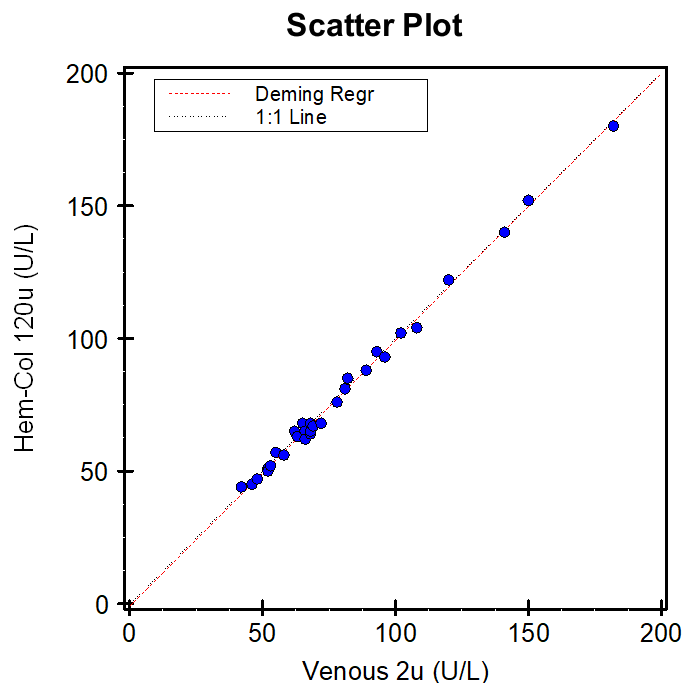

This page contains a larger, working copy of the same graphs that appear on page 1.