


## Alternate (Quantitative) Method Comparison

X Method **veneus t=0**

Y Method **Hem-Col LH t=120**

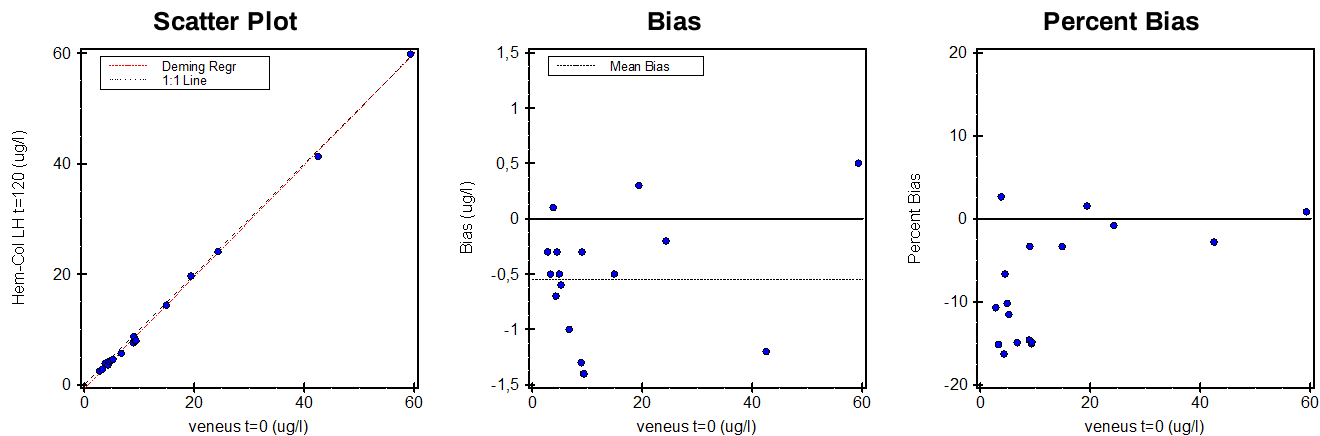

### Regression Analysis

	Deming	Regular
<b>Slope</b>	1,011 (0,992 to 1,031)	1,010 (0,991 to 1,030)
<b>Intercept</b>	-0,70 (-1,09 to -0,30)	-0,69 (-1,09 to -0,29)
<b>Std Err Est</b>	0,57	0,57

95% Confidence Intervals are shown in parentheses

### Supporting Statistics

Corr Coef (R)	0,9994	SubRange Bounds	None
Bias	-0,55 (-4,00 %)	Points (Plotted/Total)	17/22
X Mean ± SD	13,68 ± 15,48	Outliers	None
Y Mean ± SD	13,13 ± 15,65	Scatter Plot Bounds	None
Std Dev Diffs	0,57		

### Experiment Description

	X Method	Y Method
Expt Date	02 dec 2020	11 dec 2020
Rep SD	1	1
Result Ranges	2,8 to 59,3	2,5 to 59,8
Units	ug/l	ug/l
Reagent	--	--
Calibrators	--	--
Analyst	Lisanne	Lisanne
Comment		

Accepted by: \_\_\_\_\_

Signature

Date

## Alternate (Quantitative) Method Comparison

X Method venous t=0

Y Method Hem-Col LH t=120

### Experimental Results




Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias	
S00001	9,4	8,0	-1,4	<i>S00009</i>	<i>X</i>	<i>&gt;150</i>	<i>242,0</i>	S00017	3,8	3,9	0,1	
S00002	9,0	8,7	-0,3	S00010		3,3	2,8	-0,5	S00018	24,3	24,1	-0,2
S00003	4,9	4,4	-0,5	<i>S00011</i>	<i>X</i>	<i>&gt;150</i>	<i>357,2</i>	S00019	59,3	59,8	0,5	
S00004	14,9	14,4	-0,5	S00012		4,3	3,6	-0,7	S00020	19,4	19,7	0,3
S00005	6,7	5,7	-1,0	S00013		2,8	2,5	-0,3	S00021	4,5	4,2	-0,3
S00006	9,3	7,9	-1,4	<i>S00014</i>	<i>X</i>	<i>&gt;150</i>	<i>301,2</i>	<i>S00022</i>	<i>X</i>	<i>0,1</i>	<i>&lt;1,2</i>	
S00007	42,5	41,3	-1,2	S00015		8,9	7,6	-1,3				
<i>S00008</i>	<i>X</i>	<i>&gt;150</i>	<i>471,0</i>	S00016		5,2	4,6	-0,6				

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.

### Alternate (Quantitative) Method Comparison

X Method veneus t=0

Y Method Hem-Col LH t=120

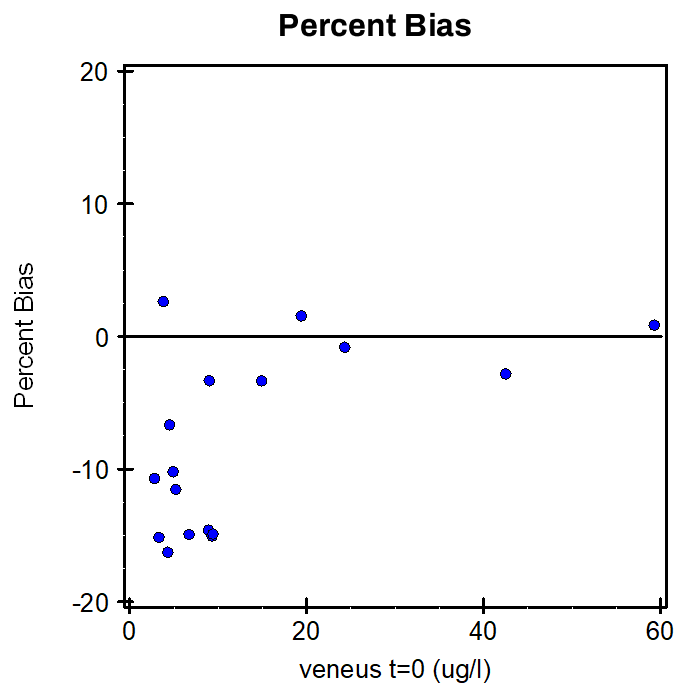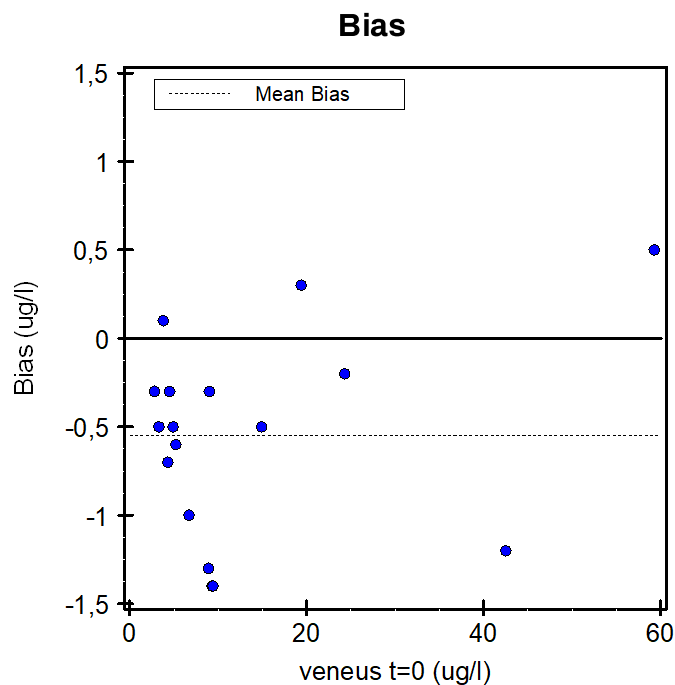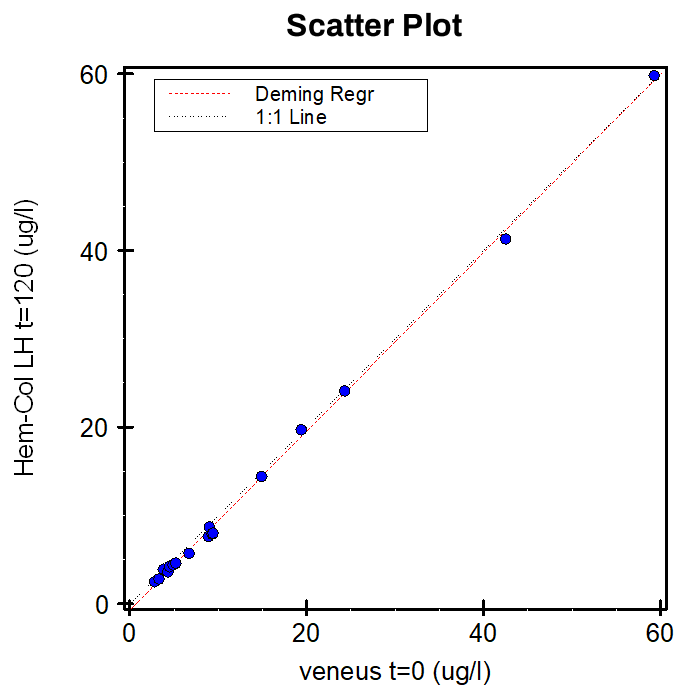

This page contains a larger, working copy of the same graphs that appear on page 1.