


Alternate (Quantitative) Method Comparison

X Method Veneus Stol 96u

Y Method Hem-Col LH 120u

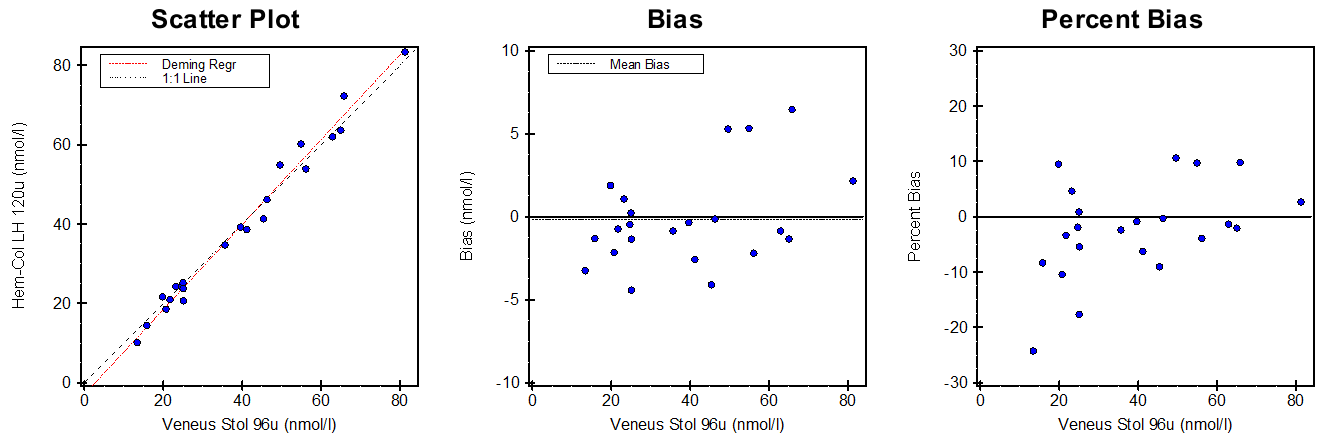

Regression Analysis

	Deming	Regular
Slope	1,071 (1,007 to 1,136)	1,062 (0,997 to 1,126)
Intercept	-2,951 (-5,745 to -0,156)	-2,578 (-5,366 to 0,210)
Std Err Est	2,724	2,718

95% Confidence Intervals are shown in parentheses

Supporting Statistics

Corr Coef (R)	0,9916	SubRange Bounds	None
Bias	-0,172 (-0,441 %)	Points (Plotted/Total)	22/22
X Mean ± SD	39,005 ± 19,209	Outliers	None
Y Mean ± SD	38,833 ± 20,566	Scatter Plot Bounds	None
Std Dev Diff	2,905		

Experiment Description

	X Method	Y Method
Expt Date	06 dec 2019	06 dec 2019
Rep SD	1	1
Result Ranges	13,40 to 81,21	10,15 to 83,36
Units	nmol/l	nmol/l
Reagent	--	--
Calibrators	--	--
Analyst	Lisanne	Lisanne
Comment		

Accepted by: _____

Signature

Date

Alternate (Quantitative) Method Comparison

X Method Veneus Stol 96u

Y Method Hem-Col LH 120u

Experimental Results

Specimen	X	Y	Bias	Specimen	X	Y	Bias	Specimen	X	Y	Bias
S00001	56,10	53,9	-2,20	S00009	20,70	18,54	-2,16	S00017	24,70	24,23	-0,47
S00002	39,60	39,25	-0,35	S00010	62,90	62,04	-0,86	S00018	45,40	41,31	-4,09
S00003	46,30	46,16	-0,14	S00011	13,40	10,15	-3,25	S00019	23,20	24,27	1,07
S00004	65,80	72,25	6,45	S00012	19,80	21,68	1,88	S00020	65,00	63,66	-1,34
S00005	49,60	54,87	5,27	S00013	25,10	23,74	-1,36	S00021	54,90	60,22	5,32
S00006	35,60	34,74	-0,86	S00014	41,20	38,62	-2,58	S00022	25,10	20,67	-4,43
S00007	25,00	25,22	0,22	S00015	21,70	20,97	-0,73				
S00008	15,80	14,48	-1,32	S00016	81,21	83,36	2,15				

Values with an "X" were excluded from the calculations. Outliers "O" were also excluded.